



1 PROPOSED EQUIPMENT LAYOUT
NOT TO SCALE


MINIMUM FOOTPRINT REQUIRED FOR A STANDARD MIDDLE ATLANTIC INTEGRATION RACK; SEE STERIS INTEGRATION DRAWINGS FOR FURTHER DETAILS

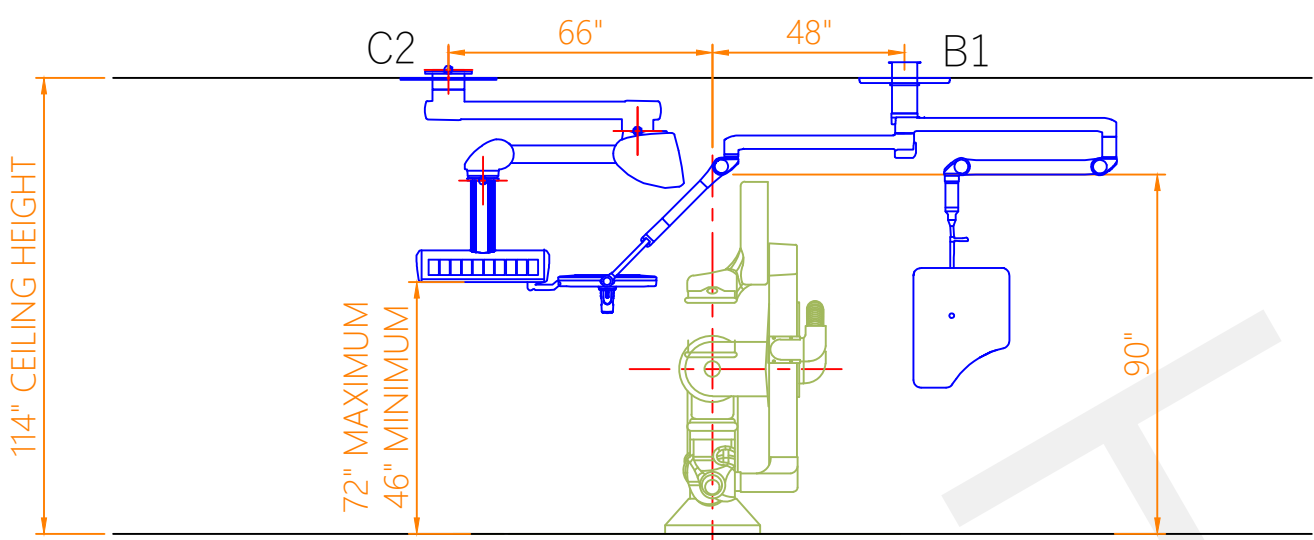

2 FOOT END EQUIPMENT ELEVATION
NOT TO SCALE

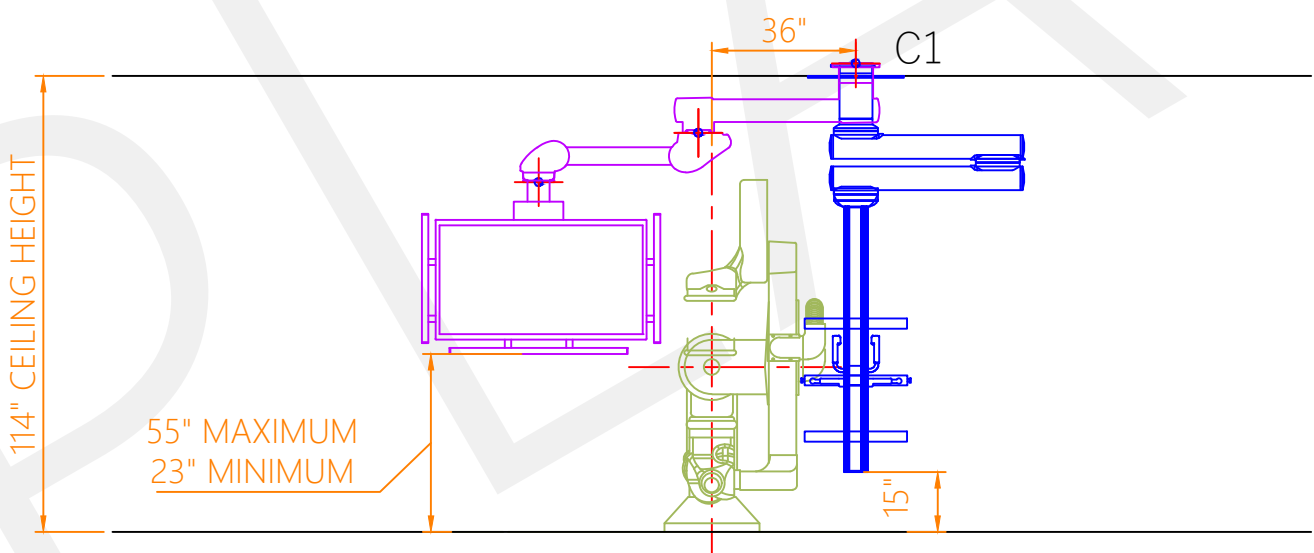

4 FOOT END EQUIPMENT ELEVATION
NOT TO SCALE

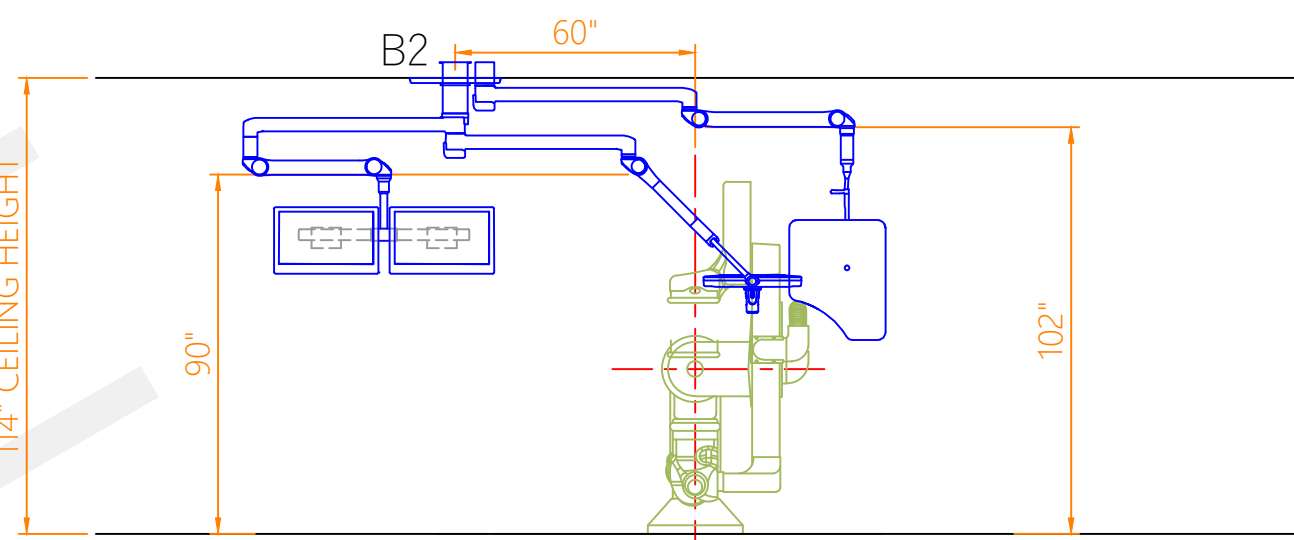

3 FOOT END EQUIPMENT ELEVATION
NOT TO SCALE

EQUIPMENT LIST		
TAG	QTY	DESCRIPTION
B1	1	A Series-Surgical Light(s) & Accessory Arm(s)
B2	1	A Series-Accessory Arm(s), Surgical Light(s) & Accessory Arm(s)
C1	1	Tandem HarmonyAIR Adj Arm Monitor Carrier - HarmonyAIR Fixed-Equipment, Monitor Carrier
C2	1	HarmonyAIR Adj Arm, Motor Supply Head-Anesthesia
K1	1	HarmonyAIR A-Series Integrated Wall Control

A SERIES LIGHT CONDUIT SCHEDULE			
FROM - TO	QUANTITY	SIZE	RESPONSIBILITY
K1 - B1	2	.75"	ELECTRICAL CONTRACTOR
K1 - B2	1	.75"	ELECTRICAL CONTRACTOR
B1 - B2	CONNECTED VIA FLEX CONDUIT INCLUDED IN SPLIT MOUNT KIT		

LIGHT CONDUIT SCHEDULE NOTES
1. 3\"/>

THIS LAYOUT IS INTENDED TO ENCOURAGE DISCUSSIONS FOR AN INTEGRATED DESIGN PROCESS.
FOR AN OPTIMIZED OPERATING ROOM DESIGN SOLUTION, PLEASE CONTACT YOUR LOCAL STERIS REPRESENTATIVE.
REFER TO THE IMAGING VENDOR FOR ALL IMAGING SYSTEM DIMENSIONS, LOCATIONS, AND REQUIREMENTS.